




The Medical Journal of Australia

Appendix

**This appendix was part of the submitted manuscript and has been peer reviewed.
It is posted as supplied by the authors.**

Appendix to: Marley JV, Oh MS, Hadgraft NT, et al. Using glycated haemoglobin testing to simplify diabetes screening in remote Aboriginal Australian health care settings. *Med J Aust* 2015; 203: 28-32. doi: 10.5694/mja14.01575.

Appendix 1. Diabetes screening used in the study and additional tests requested for participants with abnormal results[†]

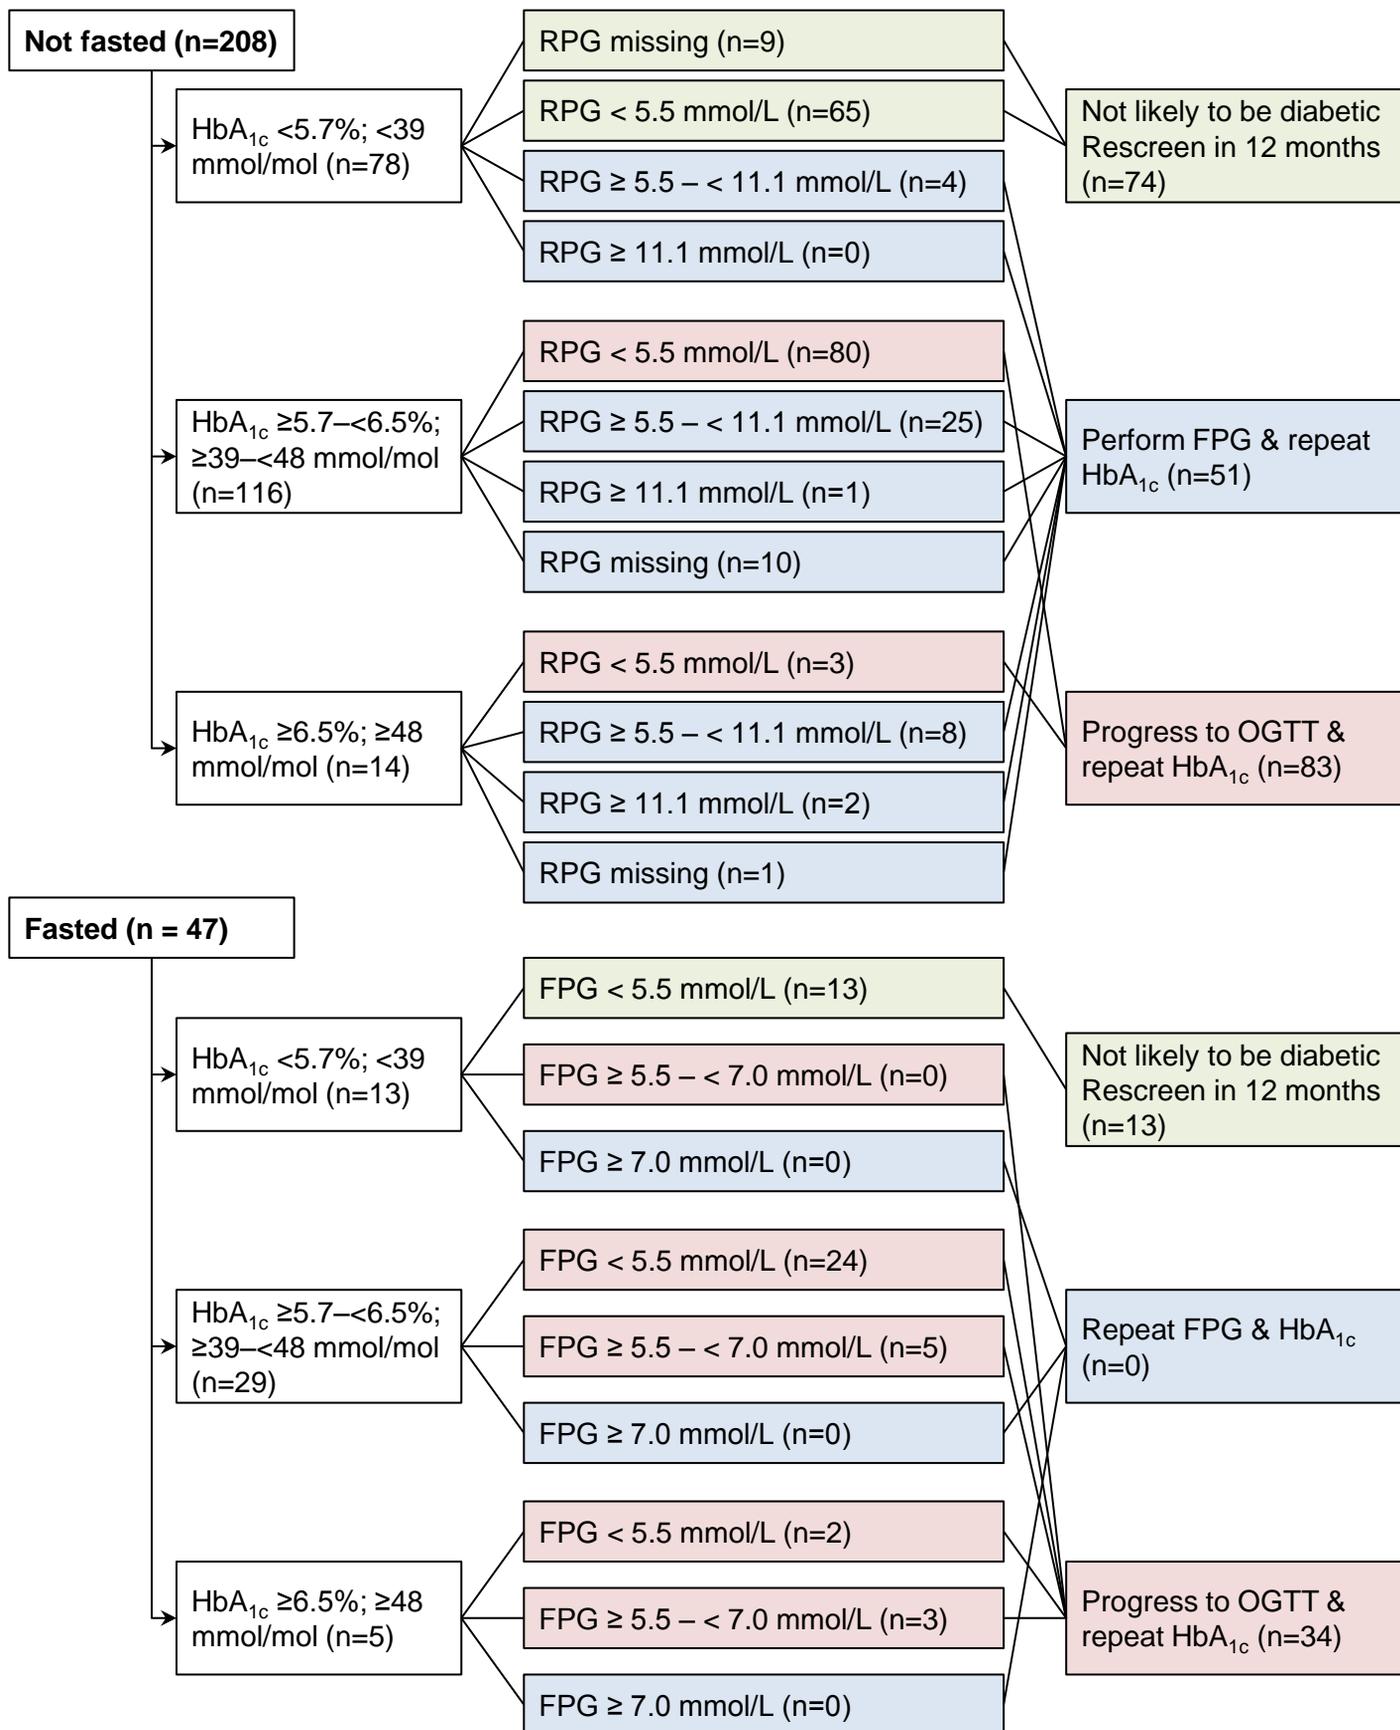

HbA_{1c} = glycated haemoglobin A1. RPG = random plasma glucose. FPG = fasting plasma glucose. OGTT = oral glucose tolerance test. POC = point-of-care.

[†] Follow-up tests requested was initially based on first laboratory (n=248) or POC HbA_{1c} measurement if the laboratory test was not completed (n=7). For participants with missing glucose tests (n=20) if both laboratory and POC HbA_{1c} measurements were normal no further tests were requested (n=9).